

MULTILAYER CAPACITOR AS AN ELECTROCHEMICAL SENSOR FOR MEASURING HYDROGEN PEROXIDE

Alvydas Radžius¹, Šarūnas Žukauskas², Arūnas Ramanavičius^{1,2}

¹Department of Physical Chemistry, Institute of Chemistry, Faculty of Chemistry and Geosciences, Vilnius University (VU), Naugarduko g. 24, LT-03225 Lt

²Department of Nanotechnology, State Research Institute Center for Physical Sciences and Technology (FTMC), Sauletekio Av. 3, LT-10257 Vilnius, Lithuania
alvydas.radzius@chgf.stud.vu.lt

Hydrogen peroxide (H_2O_2) is a widely utilized compound in laboratories, serving various purposes such as: an oxidizing agent, a reagent, or a cleaning/disinfecting agent. Unfortunately, the compound exhibits degradation, particularly in highly concentrated solutions, even at low temperatures. Traditional methods for assessing its concentration, such as titration, are time-consuming and require additional reagents.

To address this issue, an electrochemical sensor can be used to measure the concentration of H_2O_2 in solutions. In this study, a multilayer capacitor was employed as the sensing element due to its low cost of manufacturing, small physical size and compatibility with electronic systems.

Chronoamperometric measurements were performed using a three-electrode system, applying a potential of +0.3 V and introducing H_2O_2 concentrations ranging from 0.5 mmol to 5.7 mmol. The acquired chronoamperogram demonstrated distinct changes in the amperometric signal with each addition of H_2O_2 .

Using a multilayer capacitor, electrochemical measurements were successfully conducted in the solution. The resulting amperometric signal exhibited a linear dependence on the concentration of H_2O_2 , with a determined sensitivity of $3.46\text{E-}7$ A/mM. This electrochemical sensing approach offers a rapid and efficient means of quantifying H_2O_2 concentrations, presenting a valuable alternative to traditional titration methods.

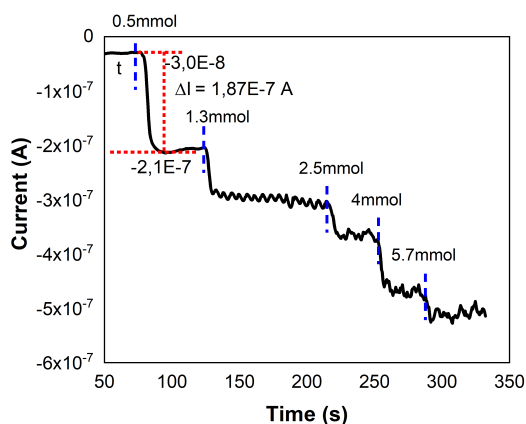


Fig. 1. Chronoamperogram obtained via a multilayer capacitor, +0.3 V in a three-electrode system, signal response from increasing the concentration of H_2O_2 in the electrolyte solution.